

# Light Measurement Report

Print date: 11-8-2025

Measurement date and time: 4-8-2025 16:35:36 – Measurement no. VFR-250804-2400-MS

Measurement tracking No. and Link: [VT250804-005306](https://www.viso-systems.com/VT250804-005306)

Operator:



## Laboratory and Equipment

Laboratory Owner and Location  
Goniospectrometer System and Type  
Sensor Name, Calibr. Date and Serial No.  
Spectrometer Manufacturer and Model

Viso Systems, Copenhagen V, Denmark  
LabSpion – Type C, horizontal  
LabSensor Model2 – 11-1-2024 – 3130191315  
Ibsen Photonics, Denmark – Freedom VIS (Custom Viso)

## Measurement Conditions

Number of C-planes and Resolution  
 $\gamma$  (gamma)-Resolution  
Test Distance  
Input Power, Power and Displ. Factors  
Input RMS Voltage and Current  
Frequency of Input Power  
Warm-up Time and Variation

12 planes – 30°  
2,5°  
2,01 m  
7,2 W – PF 0,91 – DPF 0,93  
230 V – 0,035 A  
50 Hz  
Lamp stabilized in 15 min 0 sec – 2,0%

## Tested Light Source



Product Name  
Item No. and Manufacturer  
Product Description (line 1)

812089-7W-4000K  
812089-7W-4000K – Dutchfulfillment  
LED INBOUWSPOT | MIRAN | SLIM-FIT | 5W/7W | CCT-SWITCH | ZWART

## Main Light Measurement Results

Output – Total Lumen (Up% / Down%)  
Efficiency  
Peak Intensity and Beam Angle  
Correlated Color Temperature, Target/Measured  
Color Rendering Index  
Color Rendering TM30-18  
Color Shift, CIE duv and MacAdam Steps  
Flicker

602 lm – 0,1% / 99,9%  
83 lm/W  
490 cd – 59,9°  
CCT = 4000 K / 4051 K  
CRI 83,6  
 $R_f$  84,5 –  $R_g$  96,2  
Duv 0,0013 – SDCM 1,4  
SVM 0,01 – PstLM 0,03

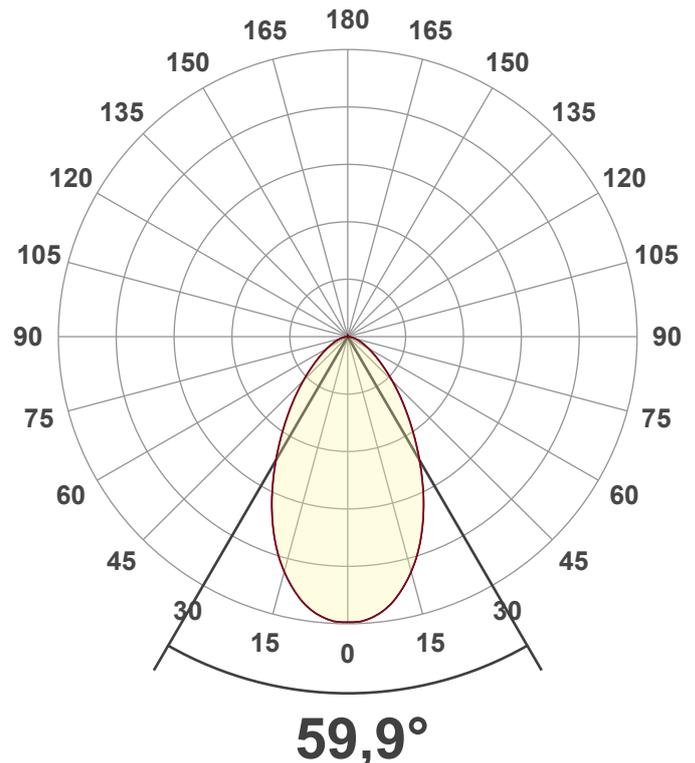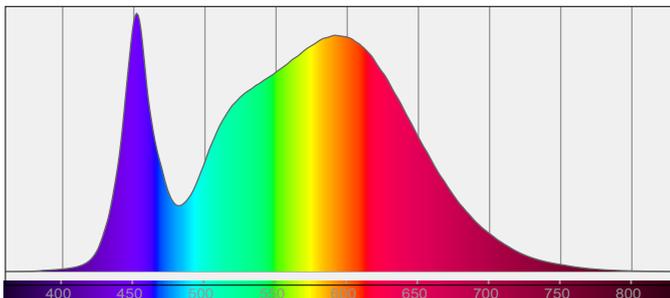

# Light Measurement Report

Print date: 11-8-2025

Measurement date and time: 4-8-2025 16:35:36 – Measurement no. VFR-250804-2400-MS


Measurement tracking No. and Link: [VT250804-005306](#)

Operator:



## Luminous Intensity diagram

Unit: 0-100% of peak intensity

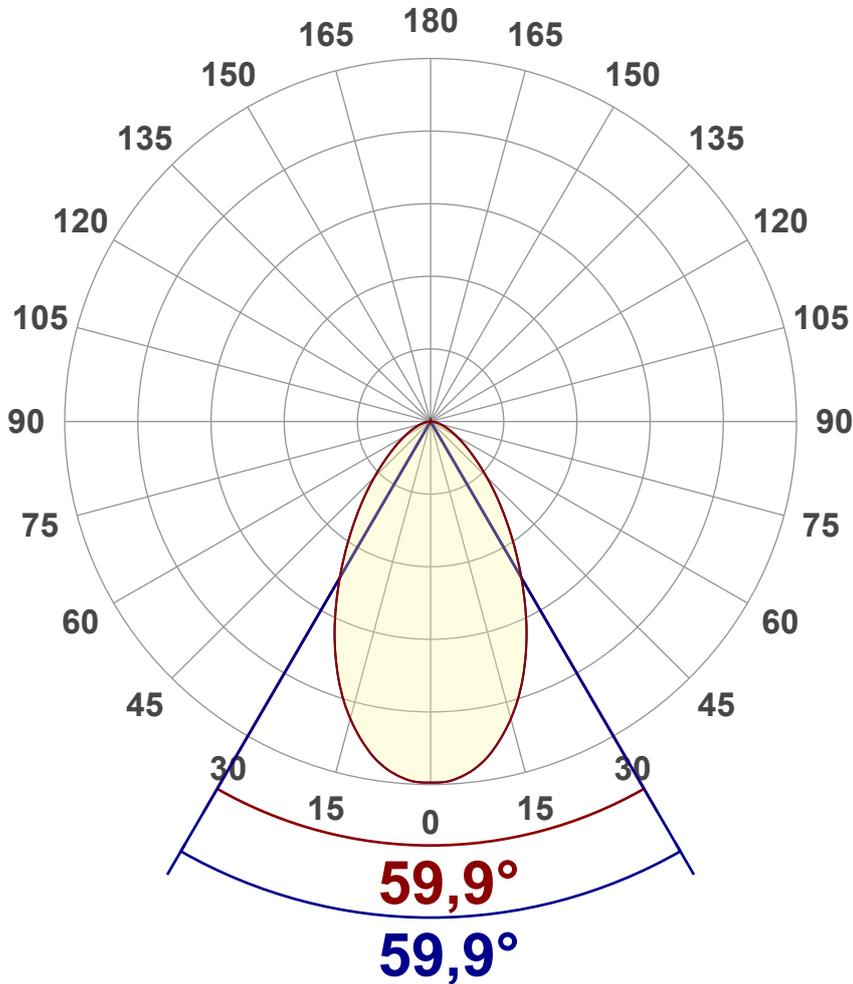

### Main Values

|                      |              |
|----------------------|--------------|
| Output (total Lumen) | 602 lm       |
| Lumen Up% / Down%    | 0,1% / 99,9% |
| Peak Intensity       | 490 cd       |
| Beam Angle (50%)     | 59,9°        |
| Beam Angle (90%)     | 59,9°        |
| Beam Angle (10%)     | 59,9°        |

### Cut-off Angle

|              |        |
|--------------|--------|
| Average 2,5% | 151,1° |
|--------------|--------|

### Field Angle

|             |        |
|-------------|--------|
| Average 10% | 114,6° |
|-------------|--------|


### Intensity Ratio

|              |       |
|--------------|-------|
| In 120° cone | 92,2% |
| In 90° cone  | 77,5% |

**C000-C180**

**C090-C270**

## Linear distribution diagram - Intensity (candela) vs $\gamma$ -angle

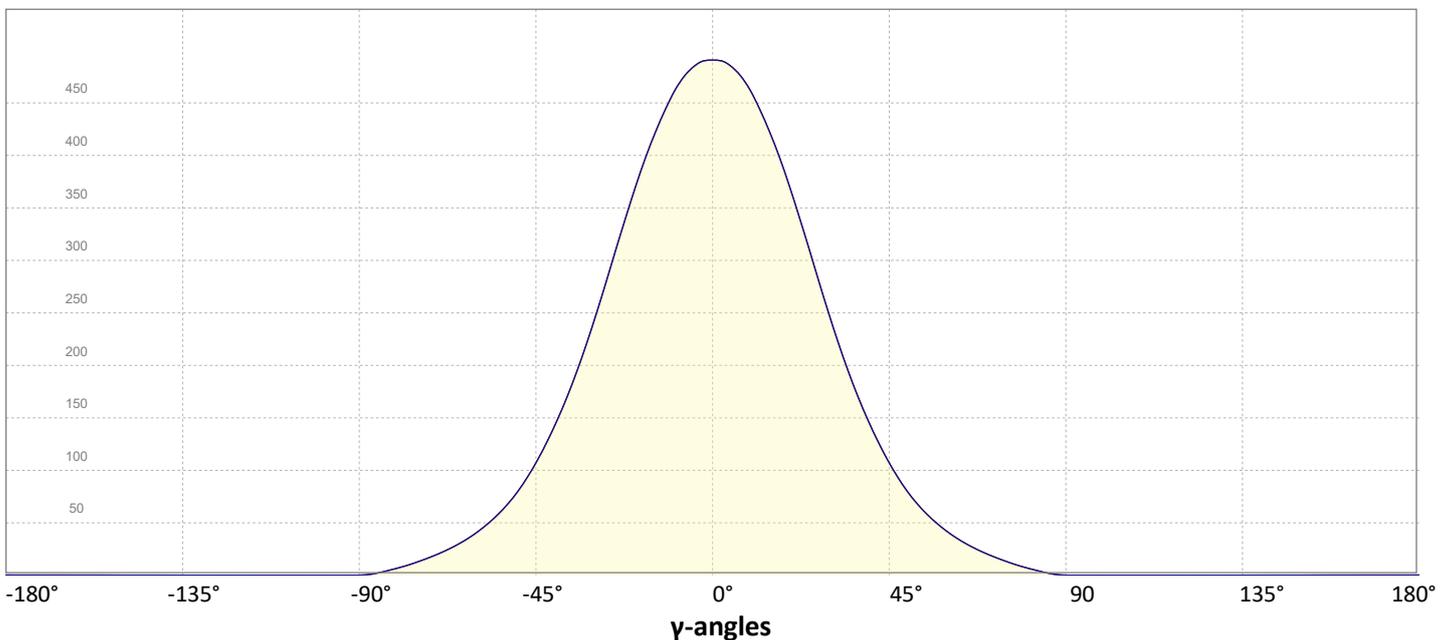

# Light Measurement Report

Print date: 11-8-2025


Measurement date and time: 4-8-2025 16:35:36 – Measurement no. VFR-250804-2400-MS

Measurement tracking No. and Link: [VT250804-005306](#)

Operator:



## Iso-intensity Diagram (Iso-candela)

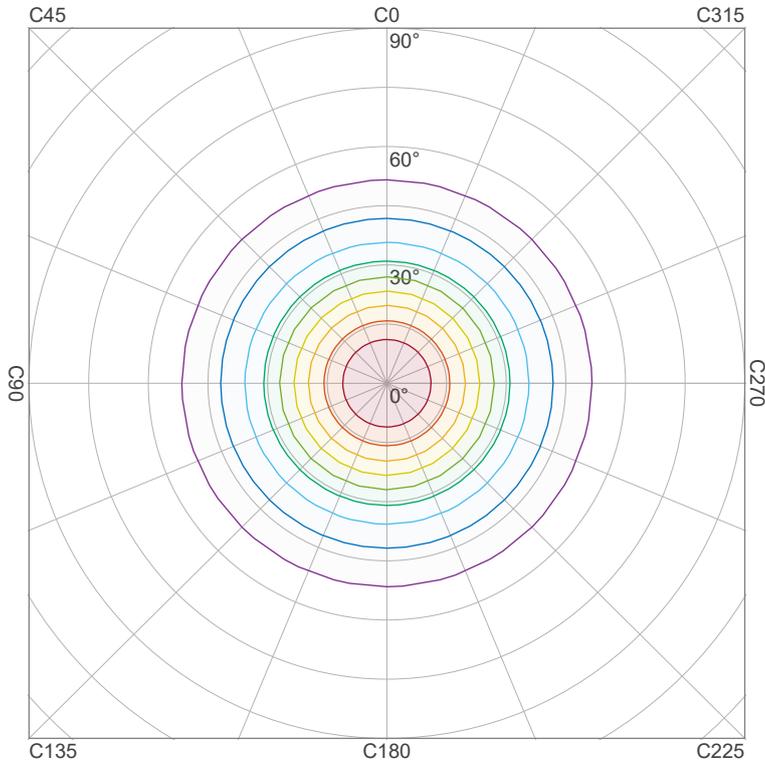


|      |          |
|------|----------|
| 90 % | 441,2 cd |
| 80 % | 392,2 cd |
| 70 % | 343,1 cd |
| 60 % | 294,1 cd |
| 50 % | 245,1 cd |
| 40 % | 196,1 cd |
| 30 % | 147,1 cd |
| 20 % | 98,0 cd  |
| 10 % | 49,0 cd  |

Peak intensity: 490,2 cd

Number of c-planes: 12

## Iso-illuminance Diagram (Iso-lux)

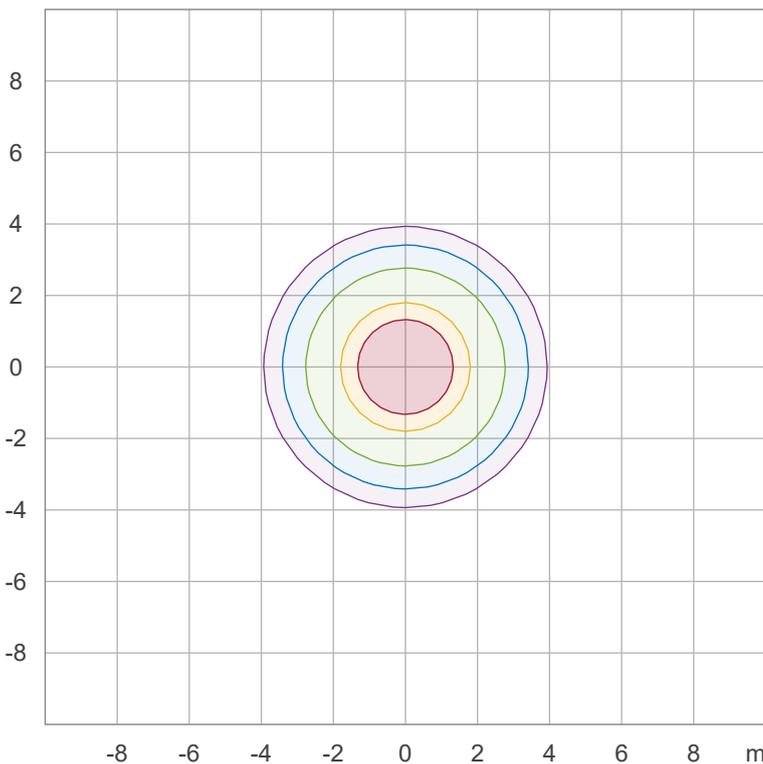

|        |         |
|--------|---------|
| 50,0 % | 27,2 lx |
| 30,0 % | 16,3 lx |
| 10,0 % | 5,4 lx  |
| 5,0 %  | 2,7 lx  |
| 3,0 %  | 1,6 lx  |

Peak illuminance: 54,5 lx

Mounting height: 3,0 m

Number of c-planes: 12

# Light Measurement Report

Print date: 11-8-2025

Measurement date and time: 4-8-2025 16:35:36 – Measurement no. VFR-250804-2400-MS

Measurement tracking No. and Link: [VT250804-005306](#)

Operator:




## Color details


Correlated Color Temperature, Target CCT = 4000 K  
 Correlated Color Temperature, Measured CCT = 4051 K  
 Color Rendering Index CRI 83,6  
 Color Rendering Index, R9 (red component) R9 = 17,1  
 Color Rendering TM30-18 R<sub>f</sub> 84,5 – R<sub>g</sub> 96,2  
 Color Quality Scale CQS = 83,0

MacAdam Steps SDCM = 1,4  
 Color coordinates CIE 1931 (x;y) = (0,381;0,377)  
 Color coordinate CIEs 1960 (u;v) = (0,225;0,334)  
 Color deviation from BBL Duv = 0,0013  
 Color coordinate CIEs 1976 (CIELUV) (u';v') = (0,225;0,502)


### CIE 1931

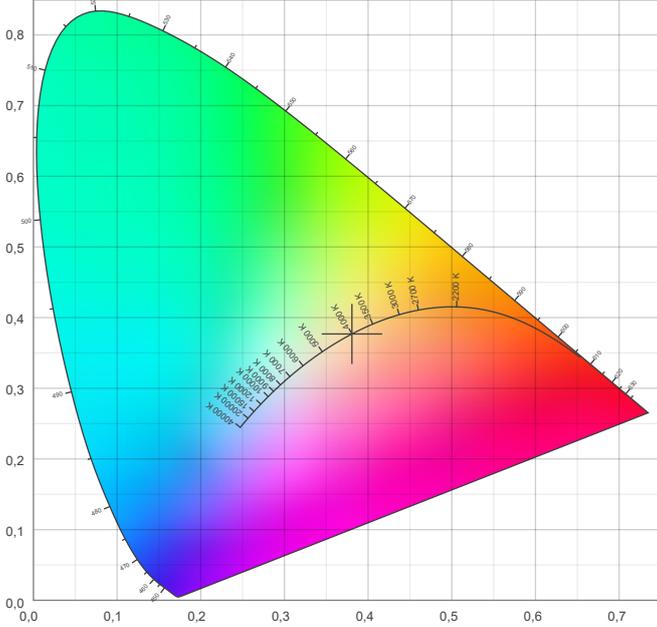

### CIE 1931 – zoomed on Planckian locus

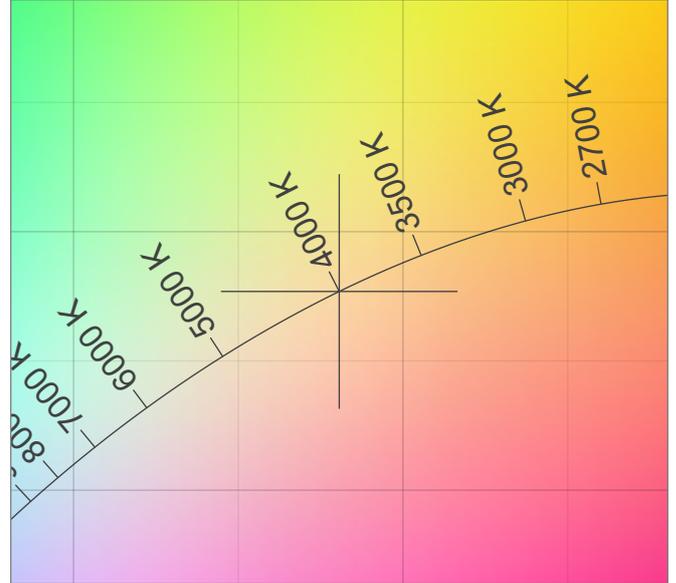


### Color Rendering Index per reference color (CIE 1995)

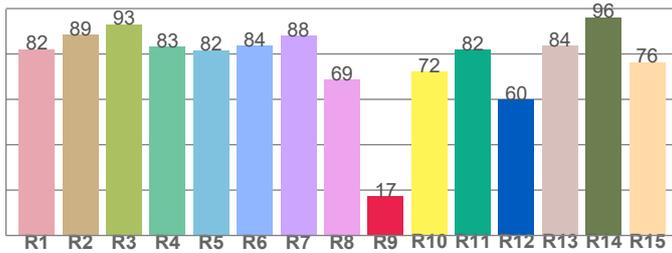


CRI R values, only R1-R8 are used to calculate final CRI value

| R1   | R2   | R3   | R4   | R5   | R6   | R7   | R8   | R9   | R10  | R11  | R12  | R13  | R14  | R15  |
|------|------|------|------|------|------|------|------|------|------|------|------|------|------|------|
| 82,1 | 88,5 | 93,1 | 83,2 | 81,6 | 83,7 | 88,1 | 68,7 | 17,1 | 72,3 | 81,8 | 59,8 | 83,6 | 96,1 | 76,3 |

### Spectral power distribution (SPD) / W/nm – 0-100%

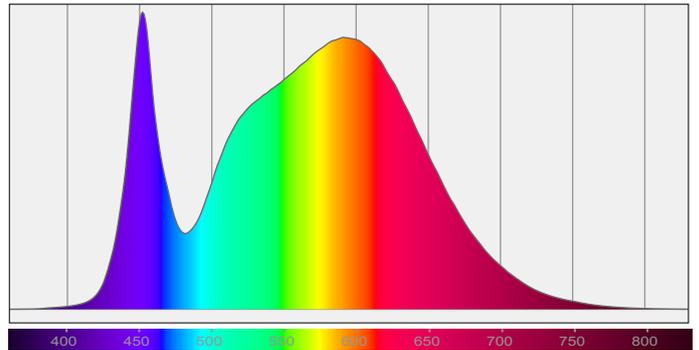


### TM30-18 Rf-values per hue bin

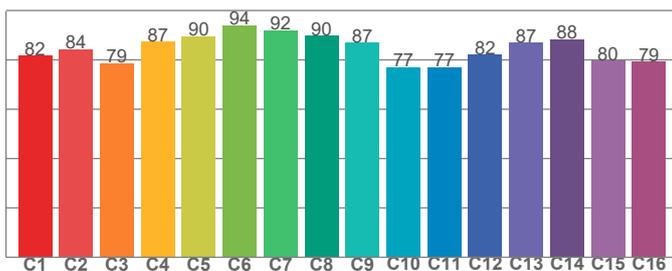

TM30 C values, 16 binned values out of total of 99 C values

| C1   | C2   | C3   | C4   | C5   | C6   | C7   | C8   | C9   | C10  | C11  | C12  | C13  | C14  | C15  | C16  |
|------|------|------|------|------|------|------|------|------|------|------|------|------|------|------|------|
| 81,7 | 84,4 | 78,7 | 87,3 | 89,6 | 94,1 | 92,0 | 89,8 | 87,1 | 77,0 | 77,0 | 82,2 | 86,9 | 88,4 | 79,7 | 79,2 |

### Color Quality Scale by reference color

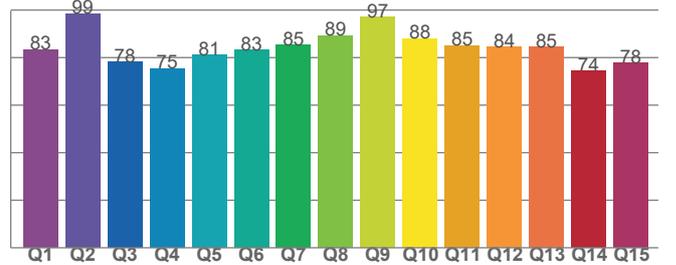

CQS Q values

| Q1   | Q2   | Q3   | Q4   | Q5   | Q6   | Q7   | Q8   | Q9   | Q10  | Q11  | Q12  | Q13  | Q14  | Q15  |
|------|------|------|------|------|------|------|------|------|------|------|------|------|------|------|
| 83,5 | 98,5 | 78,2 | 75,5 | 81,0 | 83,1 | 85,2 | 89,2 | 97,0 | 87,9 | 85,1 | 84,5 | 84,5 | 74,4 | 77,7 |

# Light Measurement Report

Print date: 11-8-2025


Measurement date and time: 4-8-2025 16:35:36 – Measurement no. VFR-250804-2400-MS

Measurement tracking No. and Link: [VT250804-005306](https://www.viso-systems.com/VT250804-005306)

Operator:



## Beam Details

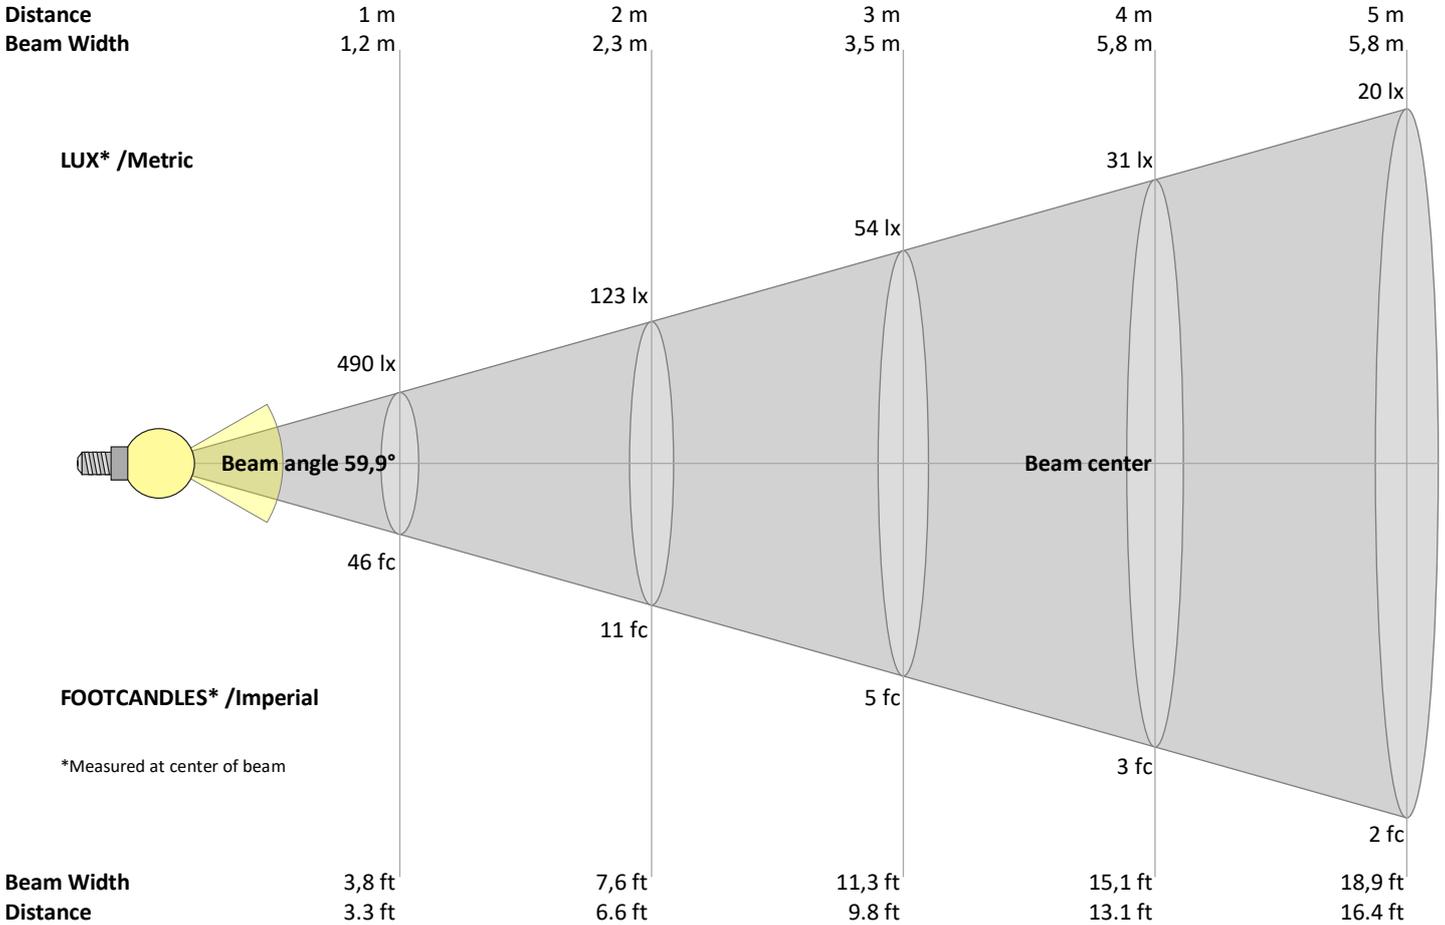

### Beam intensities from 1 – 20 m

| 1    | 2    | 3   | 4    | 5    | 6    | 7   | 8    | 9    | 10   | 11   | 12   | 13   | 14   | 15   | 16   | 17   | 18   | 19   | 20   | m   |
|------|------|-----|------|------|------|-----|------|------|------|------|------|------|------|------|------|------|------|------|------|-----|
| 3,3  | 6,6  | 9,8 | 13,1 | 16,4 | 19,7 | 23  | 26,2 | 29,5 | 32,8 | 36,1 | 39,4 | 42,7 | 45,9 | 49,2 | 52,5 | 55,8 | 59,1 | 62,3 | 65,6 | ft  |
| 490  | 123  | 54  | 31   | 20   | 14   | 10  | 8    | 6    | 5    | 4    | 3    | 3    | 3    | 2    | 2    | 2    | 2    | 1    | 1    | lux |
| 45,5 | 11,4 | 5,1 | 2,8  | 1,8  | 1,3  | 0,9 | 0,7  | 0,6  | 0,5  | 0,4  | 0,3  | 0,3  | 0,2  | 0,2  | 0,2  | 0,2  | 0,1  | 0,1  | 0,1  | fc  |

### Intensities in 0° c-plane

| 0°   | 5°  | 10° | 15° | 20° | 25° | 30° | 35° | 40° | 45° | 50° | 55° | 60° | 65° | 70° | 75° | 80° | 85° | 90° | 95° | γ        |
|------|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|----------|
| 490  | 484 | 459 | 418 | 366 | 306 | 245 | 190 | 144 | 107 | 78  | 57  | 41  | 29  | 20  | 13  | 7   | 2   | 0   | 0   | cd       |
| 100% | 99% | 94% | 85% | 75% | 62% | 50% | 39% | 29% | 22% | 16% | 12% | 8%  | 6%  | 4%  | 3%  | 1%  | 1%  | 0%  | 0%  | of 0°val |

### Intensities in 90° c-plane

| 0°   | 5°  | 10° | 15° | 20° | 25° | 30° | 35° | 40° | 45° | 50° | 55° | 60° | 65° | 70° | 75° | 80° | 85° | 90° | 95° | γ        |
|------|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|----------|
| 490  | 484 | 459 | 418 | 366 | 306 | 245 | 190 | 144 | 107 | 78  | 57  | 41  | 29  | 20  | 13  | 7   | 2   | 0   | 0   | cd       |
| 100% | 99% | 94% | 85% | 75% | 62% | 50% | 39% | 29% | 22% | 16% | 12% | 8%  | 6%  | 4%  | 3%  | 1%  | 1%  | 0%  | 0%  | of 0°val |

### Intensities in 180° c-plane

| 0°   | 5°  | 10° | 15° | 20° | 25° | 30° | 35° | 40° | 45° | 50° | 55° | 60° | 65° | 70° | 75° | 80° | 85° | 90° | 95° | γ        |
|------|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|----------|
| 490  | 484 | 459 | 418 | 366 | 306 | 245 | 190 | 144 | 107 | 78  | 57  | 41  | 29  | 20  | 13  | 7   | 2   | 0   | 0   | cd       |
| 100% | 99% | 94% | 85% | 75% | 62% | 50% | 39% | 29% | 22% | 16% | 12% | 8%  | 6%  | 4%  | 3%  | 1%  | 1%  | 0%  | 0%  | of 0°val |

### Intensities in 270° c-plane

| 0°   | 5°  | 10° | 15° | 20° | 25° | 30° | 35° | 40° | 45° | 50° | 55° | 60° | 65° | 70° | 75° | 80° | 85° | 90° | 95° | γ        |
|------|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|----------|
| 490  | 484 | 459 | 418 | 366 | 306 | 245 | 190 | 144 | 107 | 78  | 57  | 41  | 29  | 20  | 13  | 7   | 2   | 0   | 0   | cd       |
| 100% | 99% | 94% | 85% | 75% | 62% | 50% | 39% | 29% | 22% | 16% | 12% | 8%  | 6%  | 4%  | 3%  | 1%  | 1%  | 0%  | 0%  | of 0°val |

# Light Measurement Report

Print date: 11-8-2025

Measurement date and time: 4-8-2025 16:35:36 – Measurement no. VFR-250804-2400-MS

Measurement tracking No. and Link: [VT250804-005306](#)

Operator:



## Light Planning – UGR table

Uncorrected, comprehensive UGR table according to 117-1995

| Reflectances                        |           | 70   | 70   | 50   | 50   | 30   | 70   | 70   | 50   | 50   | 30   |
|-------------------------------------|-----------|--|------|------|------|------|--|------|------|------|------|
|                                     | ρ Ceiling | 70   | 70   | 50   | 50   | 30   | 70   | 70   | 50   | 50   | 30   |
|                                     | ρ Walls   | 50   | 30   | 50   | 30   | 30   | 50   | 30   | 50   | 30   | 30   |
|                                     | ρ Floor   | 20   | 20   | 20   | 20   | 20   | 20   | 20   | 20   | 20   | 20   |
| Room size                           |           | Viewed Crosswise                                   |      |      |      |      | Viewed Endwise                                   |      |      |      |      |
| H = mounting height above eye level |           | (Viewing direction orthogonal to lamp length axis) |      |      |      |      | (Viewing direction parallel to lamp length axis) |      |      |      |      |
| X                                   | Y         |  |      |      |      |      |  |      |      |      |      |
| 2H                                  | 2H        | 10,1   | 11,0 | 10,3 | 11,3 | 11,5 | 10,1   | 11,0 | 10,3 | 11,3 | 11,5 |
|                                     | 3H        | 10,6   | 11,6 | 11,0 | 11,9 | 12,1 | 10,6   | 11,6 | 11,0 | 11,9 | 12,1 |
|                                     | 4H        | 10,9   | 11,8 | 11,3 | 12,1 | 12,3 | 10,9   | 11,8 | 11,3 | 12,1 | 12,3 |
|                                     | 6H        | 11,1   | 11,9 | 11,4 | 12,2 | 12,6 | 11,1   | 11,9 | 11,4 | 12,2 | 12,6 |
|                                     | 8H        | 11,1   | 11,9 | 11,5 | 12,2 | 12,6 | 11,1   | 11,9 | 11,5 | 12,2 | 12,6 |
|                                     | 12H       | 11,1   | 11,9 | 11,5 | 12,2 | 12,6 | 11,1   | 11,9 | 11,5 | 12,2 | 12,6 |
| 4H                                  | 2H        | 10,3   | 11,2 | 10,7 | 11,5 | 11,7 | 10,3   | 11,2 | 10,7 | 11,5 | 11,7 |
|                                     | 3H        | 11,1   | 11,9 | 11,5 | 12,2 | 12,7 | 11,1   | 11,9 | 11,5 | 12,2 | 12,7 |
|                                     | 4H        | 11,4   | 12,1 | 11,8 | 12,5 | 13,0 | 11,4   | 12,1 | 11,8 | 12,5 | 13,0 |
|                                     | 6H        | 11,6   | 12,3 | 12,1 | 12,7 | 13,0 | 11,6   | 12,3 | 12,1 | 12,7 | 13,0 |
|                                     | 8H        | 11,7   | 12,3 | 12,2 | 12,7 | 13,0 | 11,7   | 12,3 | 12,2 | 12,7 | 13,0 |
|                                     | 12H       | 11,7   | 12,2 | 12,2 | 12,6 | 13,1 | 11,7   | 12,2 | 12,2 | 12,6 | 13,1 |
| 8H                                  | 4H        | 11,5   | 12,1 | 12,0 | 12,5 | 12,8 | 11,5   | 12,1 | 12,0 | 12,5 | 12,8 |
|                                     | 6H        | 11,8   | 12,3 | 12,3 | 12,7 | 13,3 | 11,8   | 12,3 | 12,3 | 12,7 | 13,3 |
|                                     | 8H        | 12,0   | 12,3 | 12,5 | 12,9 | 13,5 | 12,0   | 12,3 | 12,5 | 12,9 | 13,5 |
|                                     | 12H       | 12,0   | 12,3 | 12,6 | 12,8 | 13,4 | 12,0   | 12,3 | 12,6 | 12,8 | 13,4 |
| 12H                                 | 4H        | 11,5   | 12,0 | 12,0 | 12,4 | 12,9 | 11,5   | 12,0 | 12,0 | 12,4 | 12,9 |
|                                     | 6H        | 11,9   | 12,2 | 12,4 | 12,8 | 13,4 | 11,9   | 12,2 | 12,4 | 12,8 | 13,4 |
|                                     | 8H        | 12,0   | 12,3 | 12,6 | 12,8 | 13,4 | 12,0   | 12,3 | 12,6 | 12,8 | 13,4 |

### Variations with the observer position for the luminaire spacings, S:

|          |            |            |
|----------|------------|------------|
| S = 1.0H | 0,4 / -0,6 | 0,4 / -0,6 |
| S = 1.5H | 1,2 / -1,2 | 1,2 / -1,2 |
| S = 2.0H | 2,1 / -1,8 | 2,1 / -1,8 |

## Coefficients of Utilization

| Ceiling reflectance | 80   |     |     | 70  |     |     | 50  |     |     | 30  |     |     | 10  |     |     | 0   |     |     |
|---------------------|--|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|
| Wall reflectance    | 70   | 50  | 30  | 10  | 70  | 50  | 30  | 10  | 50  | 30  | 10  | 50  | 30  | 10  | 50  | 30  | 10  | 0   |
| Floor reflectance   | 20   | 20  | 20  | 20  | 20  | 20  | 20  | 20  | 20  | 20  | 20  | 20  | 20  | 20  | 20  | 20  | 20  | 0   |
| RCR                 | (RCR: Room Cavity Ratio)   |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
|                     | Room Values are expressed as percentage of Lumen delivered to the task surface |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |     |
| 0                   | 119  | 119 | 119 | 119 | 116 | 116 | 116 | 116 | 111 | 111 | 111 | 106 | 106 | 106 | 102 | 102 | 102 | 100 |
| 1                   | 112  | 108 | 105 | 102 | 109 | 106 | 103 | 100 | 102 | 99  | 97  | 98  | 96  | 94  | 94  | 93  | 91  | 90  |
| 2                   | 104  | 98  | 93  | 88  | 102 | 96  | 91  | 87  | 93  | 89  | 85  | 90  | 86  | 83  | 87  | 84  | 82  | 80  |
| 3                   | 97   | 89  | 83  | 78  | 95  | 88  | 82  | 77  | 85  | 80  | 76  | 82  | 78  | 74  | 80  | 76  | 73  | 71  |
| 4                   | 91   | 81  | 74  | 69  | 89  | 80  | 74  | 69  | 78  | 72  | 68  | 76  | 71  | 67  | 74  | 70  | 66  | 64  |
| 5                   | 85   | 75  | 68  | 62  | 83  | 74  | 67  | 62  | 72  | 66  | 61  | 70  | 65  | 61  | 68  | 64  | 60  | 58  |
| 6                   | 80   | 69  | 62  | 56  | 78  | 68  | 61  | 56  | 66  | 60  | 56  | 65  | 59  | 55  | 63  | 59  | 55  | 53  |
| 7                   | 75   | 64  | 57  | 52  | 74  | 63  | 56  | 51  | 62  | 56  | 51  | 60  | 55  | 51  | 59  | 54  | 50  | 49  |
| 8                   | 71   | 59  | 52  | 47  | 69  | 59  | 52  | 47  | 58  | 51  | 47  | 56  | 51  | 47  | 55  | 50  | 47  | 45  |
| 9                   | 67   | 55  | 49  | 44  | 66  | 55  | 48  | 44  | 54  | 48  | 44  | 53  | 47  | 43  | 52  | 47  | 43  | 42  |
| 10                  | 63   | 52  | 45  | 41  | 62  | 52  | 45  | 41  | 51  | 45  | 41  | 50  | 44  | 40  | 49  | 44  | 40  | 39  |

# Light Measurement Report

Print date: 11-8-2025

Measurement date and time: 4-8-2025 16:35:36 – Measurement no. VFR-250804-2400-MS

Measurement tracking No. and Link: [VT250804-005306](#)


Operator:



## Luminaire budgetary diagram

Uncorrected, comprehensive UGR table according to 117-1995

LAMPS (number of lamps)

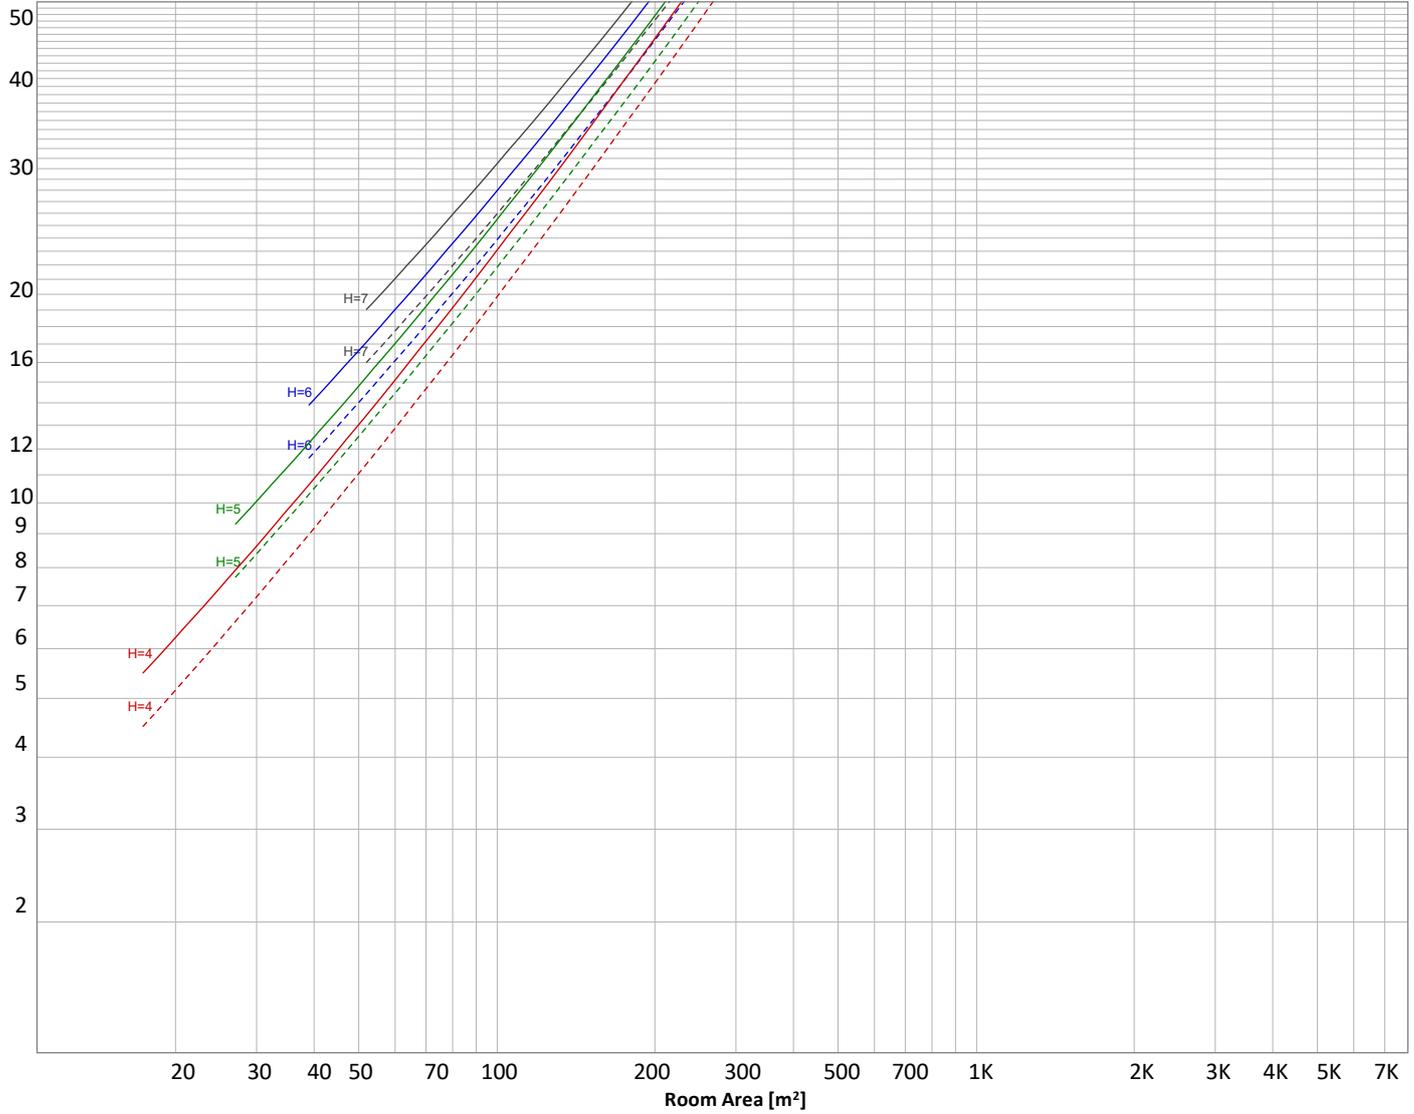

### Conditions

|   |               |           |                     |                          |                   |
|---|---------------|-----------|---------------------|--------------------------|-------------------|
| H = Room height                                   | Flux = 602 lm |           |                     |                          |                   |
| H <sub>down</sub> = Lamp distance from ceiling =  | 0.00 m        | Line type | Ceiling reflectance | ρ(%)<br>Wall reflectance | Floor reflectance |
| H <sub>work</sub> = Work area height from floor = | 0.00 m        | -----     | 70                  | 50                       | 30                |
| E <sub>work</sub> = Average lux on work area =    | 100 lx        | _____     | 50                  | 30                       | 20                |

### Zonal Lumen Summary

|          |           |           |           |           |           |           |           |           |
|----------|-----------|-----------|-----------|-----------|-----------|-----------|-----------|-----------|
| 0°-10°   | 10°-20°   | 20°-30°   | 30°-40°   | 40°-50°   | 50°-60°   | 60°-70°   | 70°-80°   | 80°-90°   |
| 45,4 lm  | 116 lm    | 140 lm    | 119 lm    | 83,3 lm   | 51,5 lm   | 29,3 lm   | 13,9 lm   | 3,10 lm   |
| 90°-100° | 100°-110° | 110°-120° | 120°-130° | 130°-140° | 140°-150° | 150°-160° | 160°-170° | 170°-180° |
| 0,063 lm | 0,057 lm  | 0,060 lm  | 0,080 lm  | 0,086 lm  | 0,091 lm  | 0,085 lm  | 0,061 lm  | 0,021 lm  |

# Light Measurement Report

Print date: 11-8-2025

Measurement date and time: 4-8-2025 16:35:36 – Measurement no. VFR-250804-2400-MS

Measurement tracking No. and Link: [VT250804-005306](#)

Operator:



## Outdoor Light Planning

### Lumen per Zone

| Zone (γ)     | Lumen         | % Total       |
|--------------|---------------|---------------|
| 0-10°        | 45 lm         | 7,5%          |
| 10-20°       | 116 lm        | 19,3%         |
| 20-30°       | 140 lm        | 23,2%         |
| 30-40°       | 119 lm        | 19,8%         |
| 40-50°       | 83 lm         | 13,8%         |
| 50-60°       | 51 lm         | 8,5%          |
| 60-70°       | 29 lm         | 4,9%          |
| 70-80°       | 14 lm         | 2,3%          |
| 80-90°       | 3 lm          | 0,5%          |
| 90-100°      | 0 lm          | 0,0%          |
| 100-110°     | 0 lm          | 0,0%          |
| 110-120°     | 0 lm          | 0,0%          |
| 120-130°     | 0 lm          | 0,0%          |
| 130-140°     | 0 lm          | 0,0%          |
| 140-150°     | 0 lm          | 0,0%          |
| 150-160°     | 0 lm          | 0,0%          |
| 160-170°     | 0 lm          | 0,0%          |
| 170-180°     | 0 lm          | 0,0%          |
| <b>Total</b> | <b>602 lm</b> | <b>100,0%</b> |

### Intensity peaks

|                |        |
|----------------|--------|
| Max intensity  | 490 cd |
| Intensity, 90° | 0 cd   |
| Intensity, 0°  | 490 cd |

### Zonal Lumen summary


| Zone (γ) | Lumen  | % Total |
|----------|--------|---------|
| 0-30°    | 301 lm | 50,1%   |
| 0-40°    | 420 lm | 69,8%   |
| 0-60°    | 555 lm | 92,2%   |
| 60-90°   | 46 lm  | 7,7%    |
| 70-100°  | 17 lm  | 2,8%    |
| 90-120°  | 0 lm   | 0,0%    |
| 0-90°    | 601 lm | 99,9%   |
| 90-180°  | 1 lm   | 0,1%    |
| 0-180°   | 602 lm | 100,0%  |

### BUG rating

|                      | Lumen  | % Total |
|----------------------|--------|---------|
| <b>Forward light</b> |        |         |
| Low(0-30°)           | 151 lm | 25,0%   |
| Medium(30-60°)       | 127 lm | 21,1%   |
| High(60-80°)         | 22 lm  | 3,6%    |
| Very high(80-90°)    | 2 lm   | 0,3%    |
| <b>Back light</b>    |        |         |
| Low(0-30°)           | 151 lm | 25,0%   |
| Medium(30-60°)       | 127 lm | 21,1%   |
| High(60-80°)         | 22 lm  | 3,6%    |
| Very high(80-90°)    | 2 lm   | 0,3%    |
| <b>Uplight</b>       |        |         |
| Low(90-100°)         | 0 lm   | 0,0%    |
| High(100-180°)       | 1 lm   | 0,1%    |

## IESNA TM-15-07 Luminaire Classification System For Outdoor Luminaires

**BUG rating B1 U1 G0**

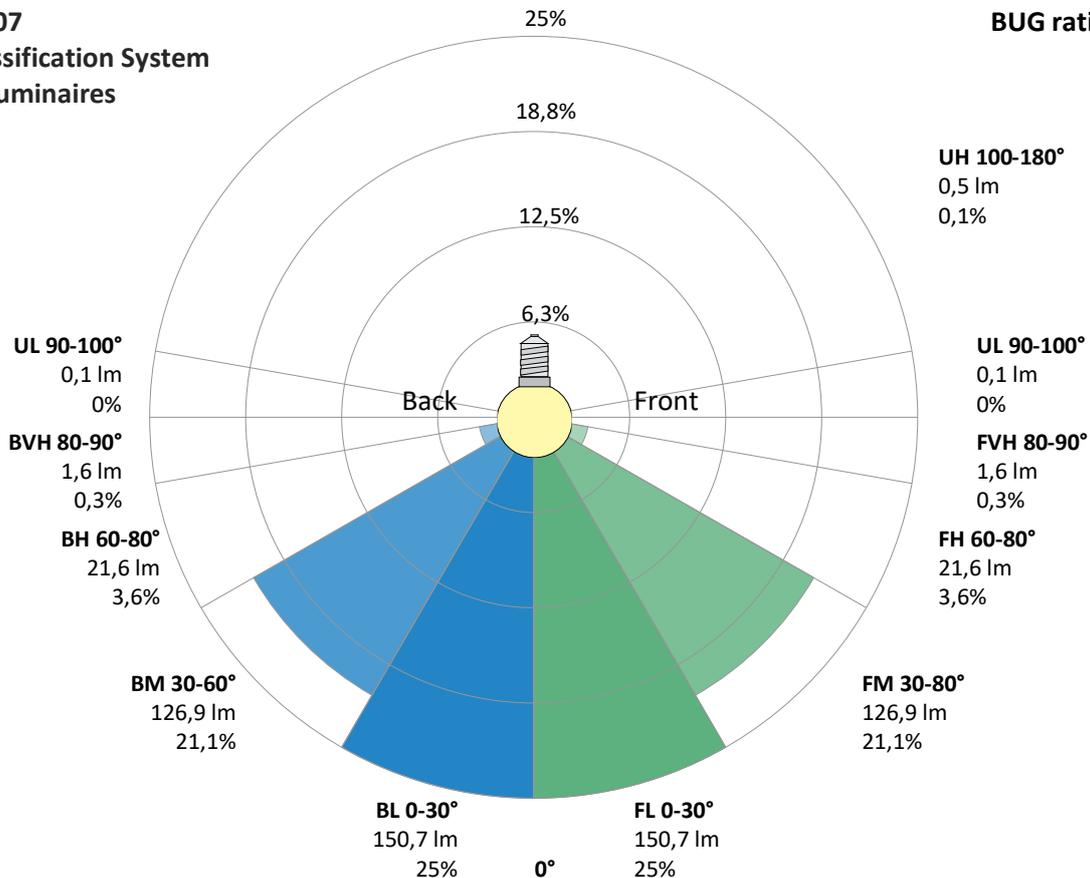

# Light Measurement Report

Print date: 11-8-2025

Measurement date and time: 4-8-2025 16:35:36 – Measurement no. VFR-250804-2400-MS

Measurement tracking No. and Link: [VT250804-005306](#)

Operator:




## Power Details


### Input Power

|   |         |
|---|---------|
| Power feed to light source                          | 7,2 W   |
| Frequency of input power                            | 50 Hz   |
| RMS Input voltage feed, $V_{RMS}$                   | 230 V   |
| RMS Input current feed, $I_{RMS}$                   | 0,035 A |
| Volt-Ampere or apparent power = $V_{RMS} * I_{RMS}$ | 7,96 VA |
| Displacement factor of AC power feed                | 0,93    |
| Power factor of AC current feed                     | 0,91    |
| Total harmonic distortion of the current            | 22,57%  |
| Total harmonic distortion of the voltage            | 0,06%   |

### Input Power Curve

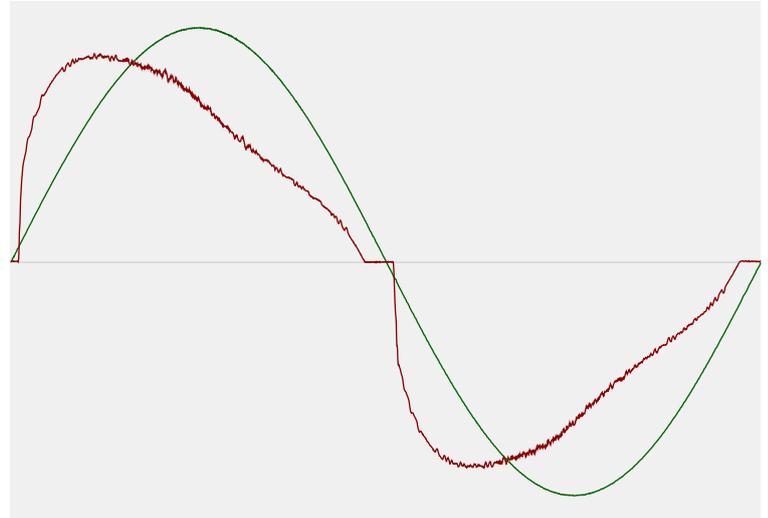

### Efficiency

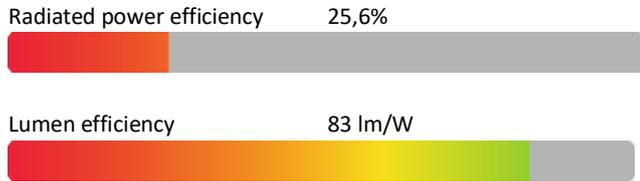

## Stabilization Details

### Warmup Conditions

|                   |        |
|-------------------|--------|
| Stable period     | 15 min |
| Stable change max | 2,0%   |
| Minimum time      | 15 min |

### Color Temperature Change

|           |        |
|-----------|--------|
| CCT start | 3997 K |
| CCT shift | +3 K   |
| CCT end   | 4000 K |


### Warmup Result

|                   |                                 |
|-------------------|---------------------------------|
| Total warmup time | Lamp stabilized in 15 min 0 sec |
| Warmup variation  | -0,2%                           |

### Output Change

|               |        |
|---------------|--------|
| Output start  | 603 lm |
| Output change | -1 lm  |
| Output end    | 602 lm |

### Stabilization Curve

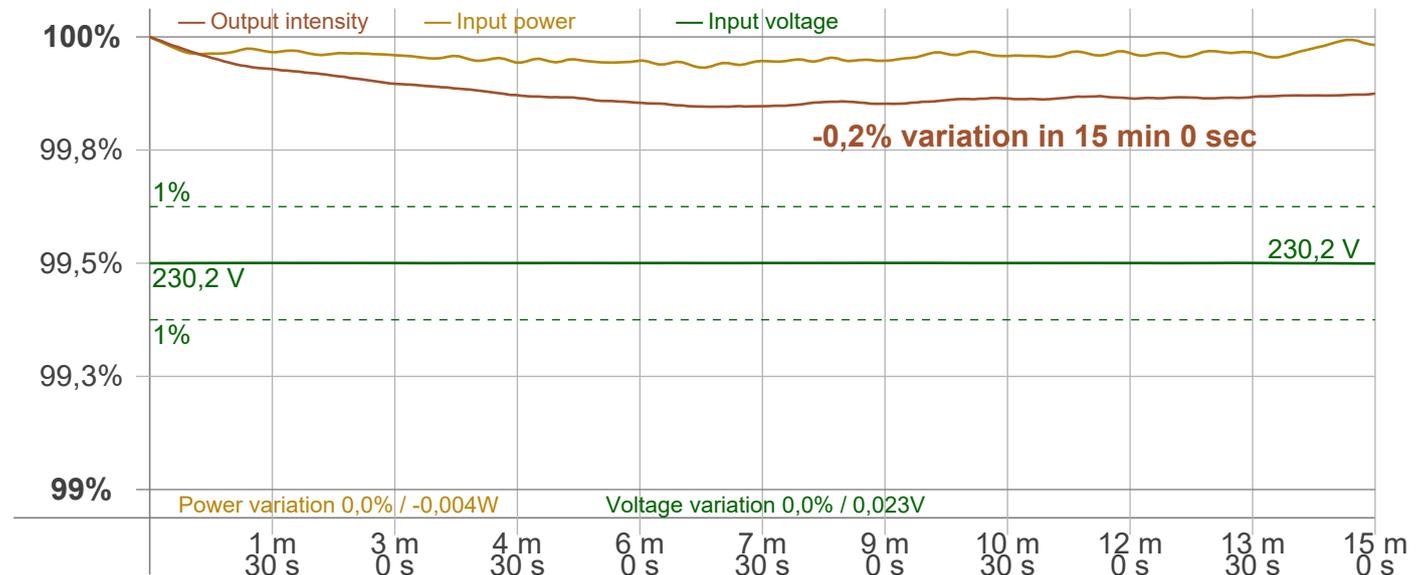

# Light Measurement Report

Print date: 11-8-2025

Measurement date and time: 4-8-2025 16:35:36 – Measurement no. VFR-250804-2400-MS

Measurement tracking No. and Link: [VT250804-005306](#)

Operator:



## Flicker /TLA details

Flicker Meter Type Viso Systems LabFlicker  
 Frequency of input power 50 Hz  
 Flicker/TLA sample rate 20000 samples/s

**Measurement time**  
 PstLM 180 sec  
 All other indices 1,2 sec

### Flicker indices according to Illuminating Engineering Society (IES)

Flicker frequency 100 Hz  
 Percent Flicker 0,21 %  
 Flicker index 0

### Flicker indices according to California Energy Commission (CEC) 2016b

JA8/10 40 Hz 0,03 %  
 JA8/10 90 Hz 0,04 %  
 JA8/10 200 Hz 0,18 %  
 JA8/10 400 Hz 0,2 %  
 JA8/10 1000 Hz 0,2 %


### TLA indices (re IEC TR 61547-1, IEC 61000-3-3 and IEC 61000-4-15)

PstLM value (F < 80 Hz) 0,03  
 SVM value (80 < F < 2000 Hz) 0,01


### Flicker indices according to Lighting Research Center (2015)

Perception metric, Assist Mp 0,01

Flicker frame (frame of one flicker period in time domain)

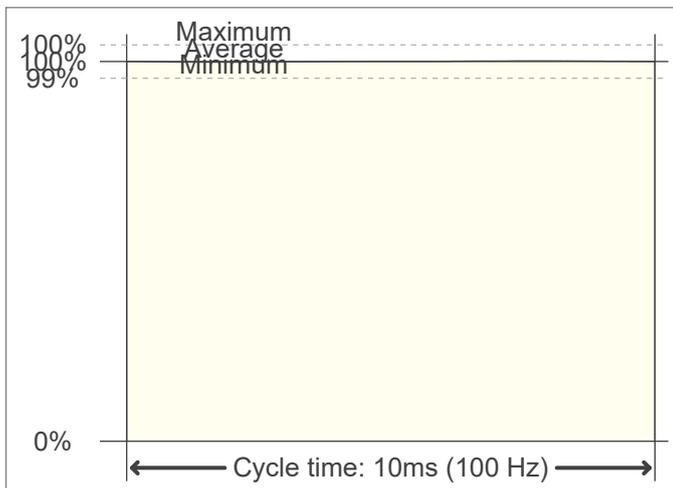

Flicker FFT (flicker curve in frequency domain)

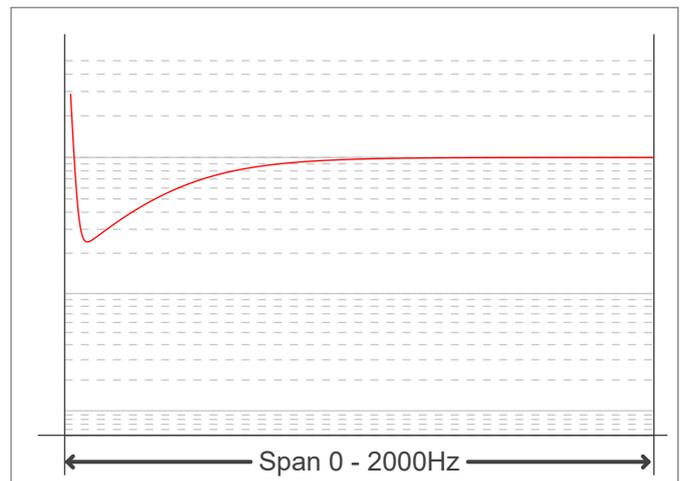

IEEE 1789 Frequency/modulation plot

